Ordering Information

Small Size (for Iliac Artery)

Proximal Graft Diameter (mm)	Distal Graft Diameter (mm)	Graft Length (mm)	Catheter Outer Diameter (fr)	Product Code
12	12	60	14	HT1212-060-0000
	12	80	14	HT1212-080-0000
14	12	80	14	HT1412-080-0000
	14	60	14	HT1414-060-0000
	14	80	14	HT1414-080-0000
16	14	80	16	HT1614-080-0000
	16	60	16	HT1616-060-0000
	16	80	16	HT1616-080-0000
	16	80	16	HT1816-080-0000
18	18	60	16	HT1818-060-0000
	18	80	16	HT1818-080-0000

Cuff


Proximal Graft Diameter (mm)	Distal Graft Diameter (mm)	Graft Length (mm)	Catheter Outer Diameter (fr)	Product Code
20	20	45	18	HT2020-045-1500
22	22			HT2222-045-1500
24	24			HT2424-045-1500
26	26			HT2626-045-1500
28	28			HT2828-045-1500
30	30	45	18	HT3030-045-2000
32	32			HT3232-045-2000
34	34			HT3434-045-2000

Aorto-Uni-Iliac


Proximal Graft Diameter (mm)	Distal Graft Diameter (mm)	Graft Length (mm)	Catheter Outer Diameter (fr)	Product Code
20	12	160	18	HT2012-160-1500
22	12	160	18	HT2212-160-1500
24	12	160	18	HT2412-160-1500
24	14	160	18	HT2414-160-1500
26	14	160	18	HT2614-160-1500
26	16	160	18	HT2616-160-1500
28	14	160	18	HT2814-160-1500
28	16	160	18	HT2816-160-1500
20	12	140	18	HT2012-140-1500
22	12	140	18	HT2212-140-1500
24	12	140	18	HT2412-140-1500
24	14	140	18	HT2414-140-1500
26	14	140	18	HT2614-140-1500
26	16	140	18	HT2616-140-1500
28	14	140	18	HT2814-140-1500
28	16	140	18	HT2816-140-1500

※ Customized products are available upon request
※ Availability may vary by local registration

Model Description

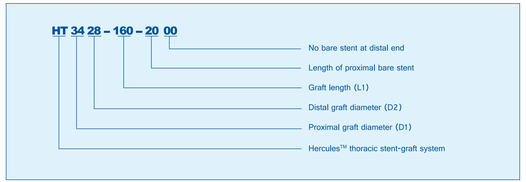

Size Range

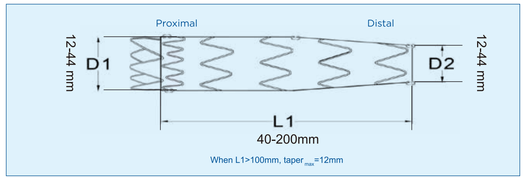


MicroPort | Endovastec™

Shanghai MicroPort Endovascular MedTech (Group) Co., Ltd.
Address:Building #1, 3399 Kangxin Rd., SIMZ Century Medicine Park, Shanghai 201318, P. R. China
Tel: +86 21 38139300 Email: xm_ib@endovastec.com Website: www.endovastec.com

All cited trademarks are the property of their respective owners in respective countries. These devices shall only be used for curing diseases on prescription by a licensed physician. Indications, contraindications, warnings, potential adverse events and directions for use can be found in Instructions for Use and product labeling supplied with each device. These devices are prohibited to promote, distribute and sell in any countries where the registration certificates or any other licenses are not obtained. This brochure is not intended for use in aforesaid countries. This brochure is only delivered to specific people for their reference, is not to be distributed widely as an advertisement. Any information may be changed without prior notice.
Not Available for Sale in the United States.
©2020 Shanghai MicroPort Endovascular MedTech (Group) Co., Ltd. All rights reserved. Version No. IB-LP-20-02

MicroPort | Endovastec™

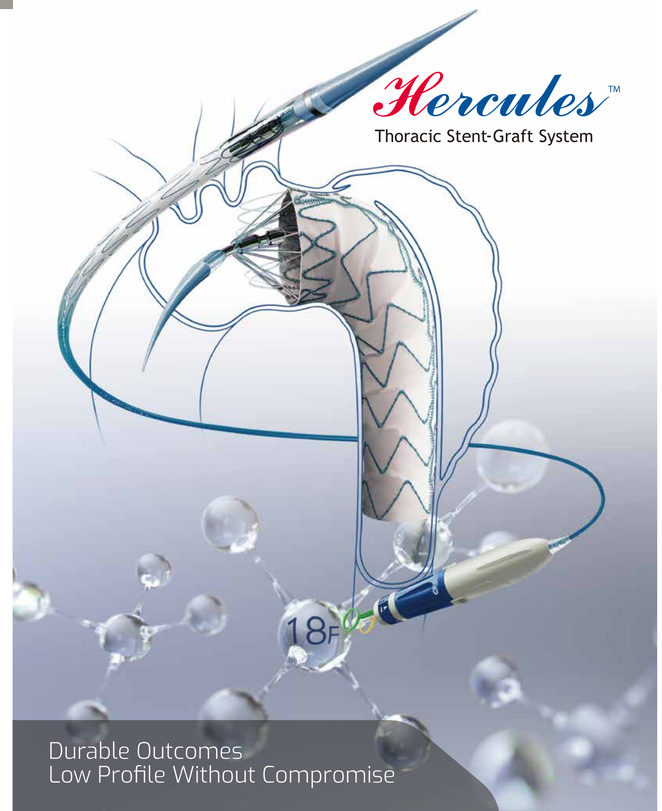

Product Code※

Straight Size


Proximal Graft Diameter (mm)	Distal Graft Diameter (mm)	Graft Length (mm)	Catheter Outer Diameter (fr)	Product Code
20	20	60	18	HT2020-060-1500
	20	80		HT2020-080-1500
	20	100		HT2020-100-1500
22	22	60		HT2222-060-1500
	22	80		HT2222-080-1500
	22	100		HT2222-100-1500
24	24	60		HT2424-060-1500
	24	80		HT2424-080-1500
	24	100		HT2424-100-1500
26	26	60		HT2626-060-1500
	26	80		HT2626-080-1500
	26	100		HT2626-100-1500
28	28	60		HT2828-060-1500
	28	80		HT2828-080-1500
	28	100		HT2828-100-1500
30	30	60		HT3030-060-2000
	30	80		HT3030-080-2000
	30	100		HT3030-100-2000
32	32	60	18	HT3232-060-2000
	32	80		HT3232-080-2000
	32	100		HT3232-100-2000
34	34	60	18	HT3434-060-2000
	34	80		HT3434-080-2000
	34	100		HT3434-100-2000
36	36	60	18	HT3636-060-2000
	36	80		HT3636-080-2000
	36	100		HT3636-100-2000
38	38	80	20	HT3838-080-2000
	38	100		HT3838-100-2000
40	40	80	20	HT4040-080-2000
	40	100		HT4040-100-2000
42	42	80	20	HT4242-080-2000
	42	100		HT4242-100-2000
44	44	80	20	HT4444-080-2000
	44	100		HT4444-100-2000

Tapered Size (4mm)

Proximal Graft Diameter (mm)	Distal Graft Diameter (mm)	Graft Length (mm)	Catheter Outer Diameter (fr)	Product Code
30	26	140	18	HT3026-140-2000
32	28	140	18	HT3228-140-2000
34	30	140	18	HT3430-140-2000
36	32	140	18	HT3632-140-2000
38	34	140	20	HT3834-140-2000
30	26	160	18	HT3026-160-2000
32	28	160	18	HT3228-160-2000
34	30	160	18	HT3430-160-2000
36	32	160	18	HT3632-160-2000
38	34	160	20	HT3834-160-2000
40	36	160	20	HT4036-160-2000
42	38	160	20	HT4238-160-2000
30	26	180	18	HT3026-180-2000
32	28	180	18	HT3228-180-2000
34	30	180	18	HT3430-180-2000
36	32	180	18	HT3632-180-2000
38	34	180	20	HT3834-180-2000
40	36	180	20	HT4036-180-2000
42	38	180	20	HT4238-180-2000
30	26	200	18	HT3026-200-2000
32	28	200	18	HT3228-200-2000
34	30	200	18	HT3430-200-2000
36	32	200	18	HT3632-200-2000
38	34	200	20	HT3834-200-2000
40	36	200	20	HT4036-200-2000
42	38	200	20	HT4238-200-2000

Durable Outcomes, Low Profile Without Compromise

Low Profile Sheath With Hydrophilic Coating

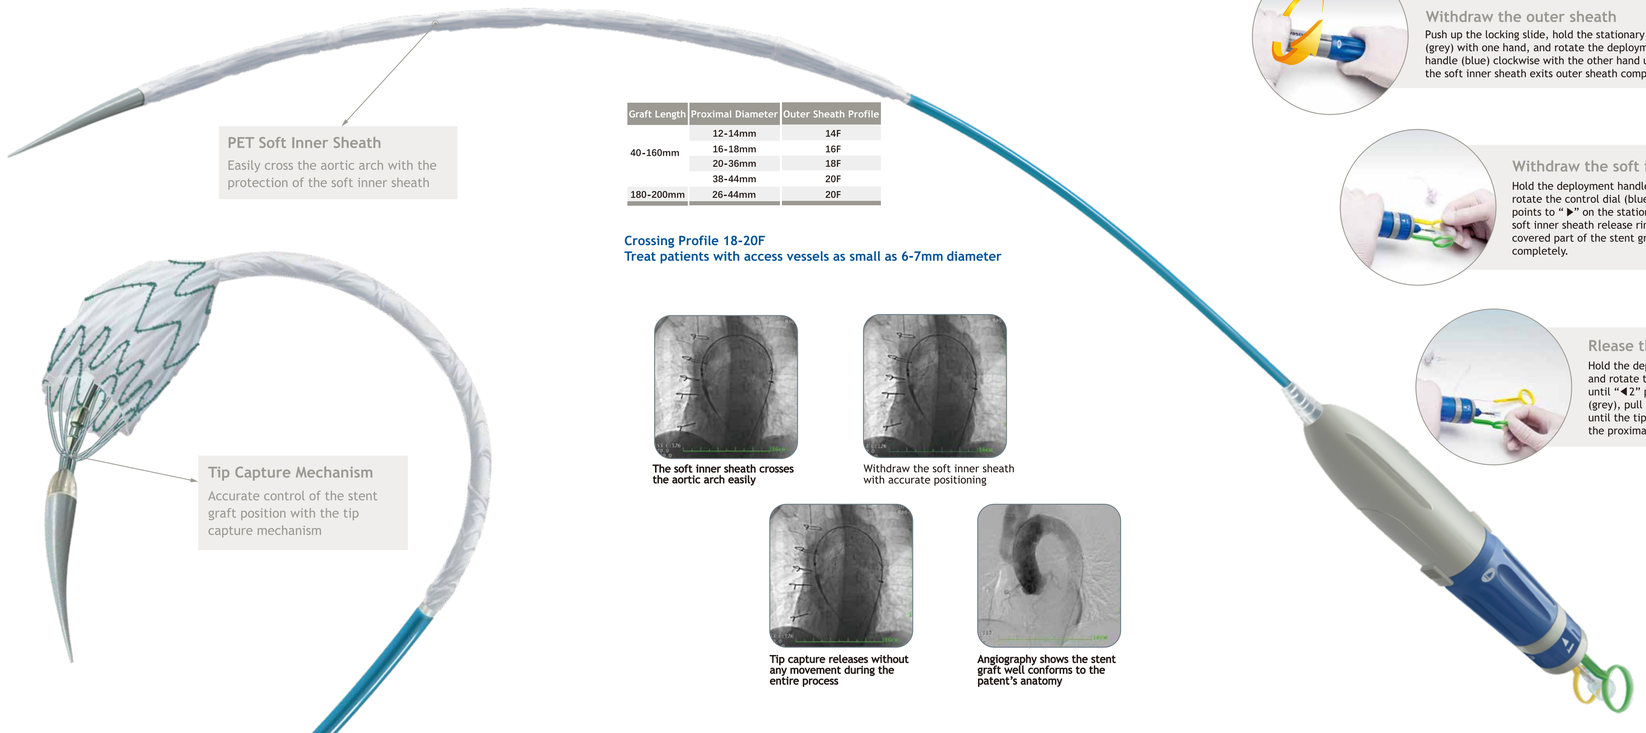

PET Soft Inner Sheath
Easily cross the aortic arch with the protection of the soft inner sheath

Tip Capture Mechanism
Accurate control of the stent graft position with the tip capture mechanism

Graft Length	Proximal Diameter	Outer Sheath Profile
40-160mm	12-14mm	14F
	16-18mm	16F
	20-36mm	18F
	38-44mm	20F
180-200mm	26-44mm	20F

Crossing Profile 18-20F
Treat patients with access vessels as small as 6-7mm diameter

The soft inner sheath crosses the aortic arch easily

Withdraw the soft inner sheath with accurate positioning

Tip capture releases without any movement during the entire process

Angiography shows the stent graft well conforms to the patent's anatomy

Deployment Process

Withdraw the outer sheath
Push up the locking slide, hold the stationary grip (grey) with one hand, and rotate the deployment handle (blue) clockwise with the other hand until the soft inner sheath exits outer sheath completely.

Withdraw the soft inner sheath
Hold the deployment handle (blue) stationary, and rotate the control dial (blue) clockwise until "◀1" points to "▶" on the stationary dial (grey), pull the soft inner sheath release ring (yellow) until the covered part of the stent graft is deployed completely.

Rlease the bare stent
Hold the deployment handle (blue) stationary, and rotate the control dial (blue) clockwise until "◀2" points to "▶" on the stationary dial (grey), pull the tip capture release ring (green) until the tip capture mechanism is released and the proximal bare stent is completely open.

Stent-Graft Design



Nitinol Wire
-Superelastic shape memory alloy
-Stable radial strength



PET Graft
-Great biocompatibility
-Thin thickness
-Superior strength
-Low blood leakage

Mini Spring
-Proprietary
-Increased radial strength
-Perfect match with the artery
-Decreased endoleak risk

Main-Body Stent
-Height-mutative
-Readily conforming to the contours of the aorta
-Kinking-free

2-10mm Multi-taper Design adjust more dissection

	Tapper
Hercules® Low-Profile	2/4/6/8/10mm
Competitor1	4mm
Competitor2	4mm
Competitor3	/