

CH15465_MODIFICATION ROW BROCHURE PCP.indd 1 28/09/2023 11:02

CH15465_MODIFICATION ROW BROCHURE PCP.indd 2 28/09/2023 11:02

CONTENT

2 DIXI MEDICAL

3 SEEG (Stereoelectroencephalography)

4 MICRODEEP®
SEEG ELECTRODES

7 IMPLANTATION TOOLS

11 CBL CONNECTION CABLES

12 REMOVAL TOOLS

14 THERMOCOAGULATION

16 INTRAOPERATIVE CORTEX STRIP
/GRID ELECTRODES

20 DIXI MEDICAL SUPPORT

DIXI Medical is not responsible for the misuse of its products. Carefully read the information provided in the "Instructions for Use" (IFU) and product labeling. If you have questions regarding this material, please contact your DIXI Medical representative. Drawings and pictures are for reference only. All technical specifications may be modified without notice. For more information contact: info@diximedical.com

CH15465_MODIFICATION ROW BROCHURE PCP.indd 3 28/09/2023 11:02

DIXI medical

For more than 40 years, DIXI medical never ceased to innovate and improve its intracerebral electrodes and implantation accessories, working hand in hand with neurosurgeons, neurologists and scientists from all around the world. The factory and its 100 highly skilled and knowledgeable employees are based since the beginning in Besançon, France.

Back in the 1970s, a group of physicians and scientists from Rennes University Hospital visited a fair focusing on the watchmaking and microtechniques industries in Besançon in the hope of finding new partners to develop tools for neurosurgery.

Prof. Scarabin and his team worked on SEEG (Stereo-Electro-Encephalography), a new surgical technique to treat drug-resistant epilepsy developed in the 1960s at St-Anne hospital in Paris with Prof. Talairach. The collaboration between the neuroscientists and the precision industry experts blossomed over the years.

DIXI, a family-owned company founded in 1904 in Le Locle, Switzerland, specialized in precision industry, microtechnology and neurology, took over in 1988. In the 1990s, the industrial production of the SEEG electrodes and implantation tools started. The French company slowly expanded internationally while DIXI medical products have been FDA approved since November 2017.

CH15465_MODIFICATION ROW BROCHURE PCP.indd 4 28/09/2023 11:02

SEEG (Stereoelectroencephalography)

SEEG is a minimally invasive diagnostic procedure for drug-resistant focal epilepsy. The objective is to identify the epileptic foci. To do so, electrodes are implanted in predefined brain parts to record electrical activities and epileptic seizures. The patient stays a few days (maximum 29) in the hospital under EEG monitoring and video recording surveillance. Thermocoagulation may be performed in some cases. The data collected is analyzed to refine the diagnosis and plan the following treatment options.

SEEG vs. Subdural Strips and Grids

While subdural strip and grids electrodes provide a large coverage over the bare surface of the cerebral cortex, they do not reach deeper brain structures (e.g., hippocampus or insula). By comparison, SEEG electrodes can enable monitoring of superficial and deep cortical structures and facilitate the electrical stimulation mapping of these regions. Thus, they allow testing hypotheses about the localization of the seizure onset zone in three dimensions and studying the seizure network in detail[1]. DIXI medical SEEG electrodes also offer the possibility to perform thermocoagulation.

Several reports document the benefits and risks of SEEG electrodes relative to the subdural ones. These reports demonstrate that SEEG electrodes allow targeting deeply situated foci with a non-inferior safety profile to subdural electrodes and comparable seizure outcome[2-5].

[1] *Gholipour, T., Koubeissi, M. Z. & Shields, D. C. Stereotactic electroencephalography. Clin. Neurol. Neurosurg. 189, 105640 (2020).*
[2] *Joswig, H. et al. Stereoelectroencephalography Versus Subdural Strip Electrode Implantations: Feasibility, Complications, and Outcomes in 500 Intracranial Monitoring Cases for Drug-Resistant Epilepsy. Neurosurgery 87, E23–E30 (2020).*
[3] *Remick, M., Ibrahim, G. M., Mansouri, A. & Abel, T. J. Patient phenotypes and clinical outcomes in invasive monitoring for epilepsy: An individual patient data meta-analysis. Epilepsy Behav. 102, 106652 (2020).*
[4] *Toth, M. et al. Surgical outcomes related to invasive EEG monitoring with subdural grids or depth electrodes in adults: A systematic review and meta-analysis. Seizure 70, 12–19 (2019).*
[5] *Yang, M. et al. A Retrospective Analysis of Stereoelectroencephalography and Subdural Electroencephalography for Preoperative Evaluation of Intractable Epilepsy. Stereotact. Funct. Neurosurg. 95, 13–20 (2017).*

CH15465_MODIFICATION ROW BROCHURE PCP.indd 5 28/09/2023 11:02

MICRODEEP®

SEEG ELECTRODES

For SEEG exploration, functional mapping
and thermocoagulation of epileptic foci



Class III, CE mark issued by GMED 0459

Single-use sterile material


CH15465_MODIFICATION ROW BROCHURE PCP.indd 6 28/09/2023 11:02

MICRODEEP® is a multi-contact flexi-rigid intracerebral electrode, with a diameter of 0.8 mm and a hemispherical tip.

The active part is hand polished for an optimized smooth surface.


- Diameter 0.8 mm
- Platinum / Iridium
- From 5 to 18 contacts
- Active exploration length ranges from 16 mm to 80.5 mm
- Suitable for thermocoagulation[1]
- Proprietary cap designed to prevent the electrode from moving to ensure a good seal and to serve as a depth maker
- Total length: 100 cm
- Connection cables CBL (page 12)

Reference	Nr of contacts	Dimensions (mm)		
		Lt	Lc	Li
D08-05AM	5	16	2	1.5
D08-08AM	8	26.5	2	1.5
D08-10AM	10	33.5	2	1.5
D08-12AM	12	40.5	2	1.5
D08-15AM	15	51	2	1.5
D08-18AM	18	61.5	2	1.5



To optimize the recording of deep surfaces and avoid losing contacts in white matter, three long electrodes are designed with specific spacing in between groups of contacts.


Reference	Nr of contacts	Dimensions (mm)			
		Lt	Lc	Li	Lsi
D08-15BM	15 (3x5)	62	2	1.5	7
D08-15CM	15 (3x5)	70	2	1.5	11
D08-18CM	18 (3x6)	80.5	2	1.5	11

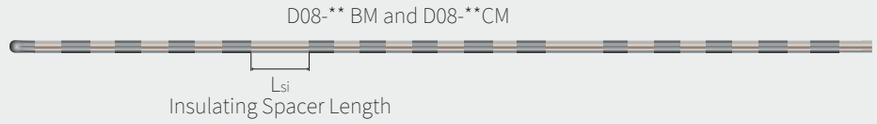



[1] *Please contact your local representatives for more information on thermocoagulation.*


CH15465_MODIFICATION ROW BROCHURE PCP.indd 7 28/09/2023 11:02

MICRODEEP® SEEG electrodes

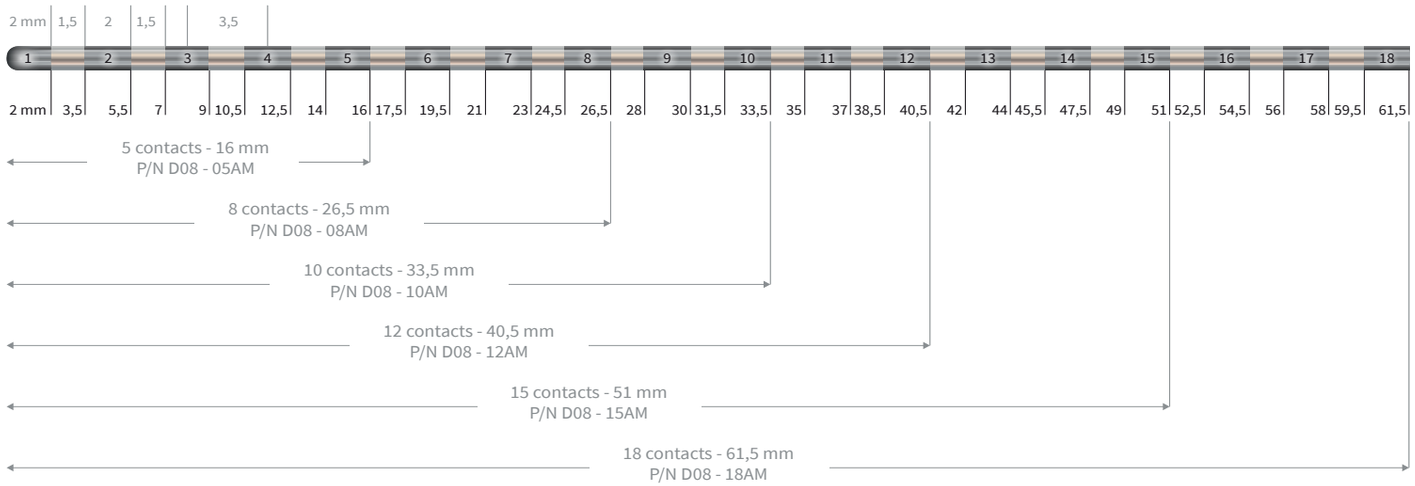

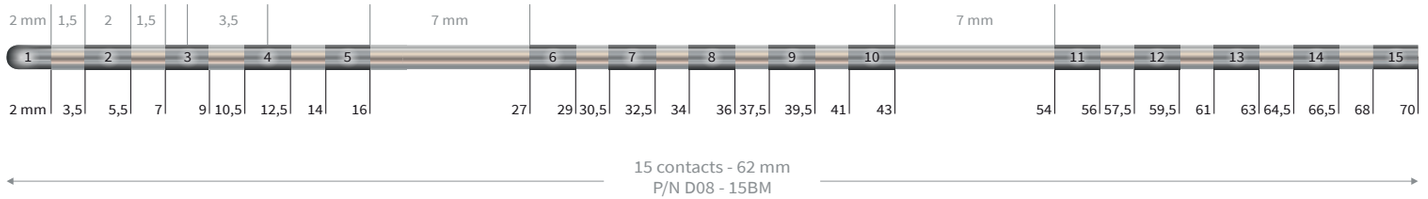

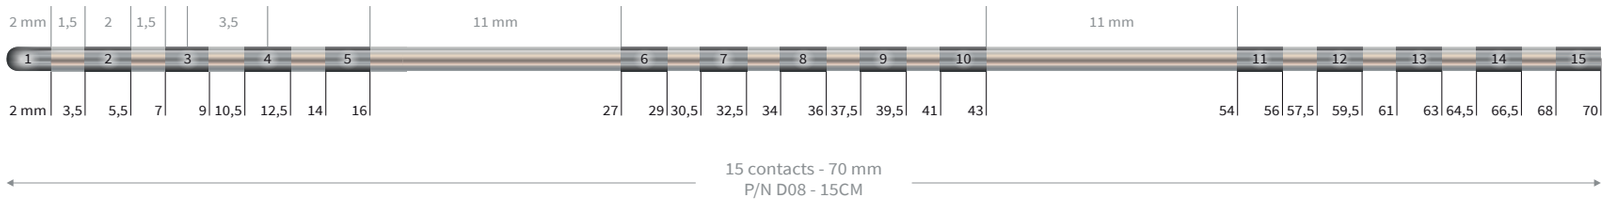

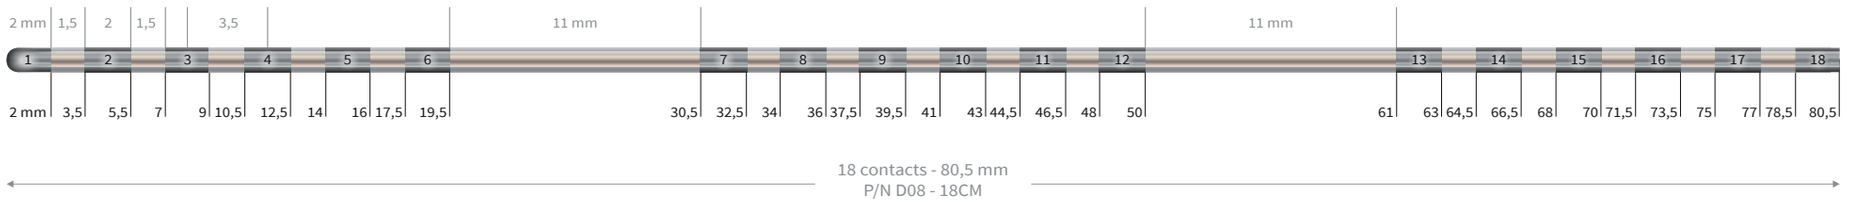

FOR REFERENCES ONLY
Extracted from document number: 5100.XX00.500A

CH15465_MODIFICATION ROW BROCHURE PCP.indd 8 28/09/2023 11:02

IMPLANTATION TOOLS

DIXI medical optimizes the SEEG flow in the OR by offering implantation tools to be used in sequential order to provide the best and most accurate implantation.

All implantation tools have an outer diameter of 2.45 mm and fit through a guide tube of min 2.5 mm[1].

BONE STARTER
ACS-745

Class I, CE mark
Delivered Non-sterile

- To pierce the skin and mark the skull before drilling




ACS-745

SLIDING RULER
ACS-750

Class Im, CE mark issued by GMED 0459
Delivered Non-sterile

- To measure the length of DIXI medical implantation accessories

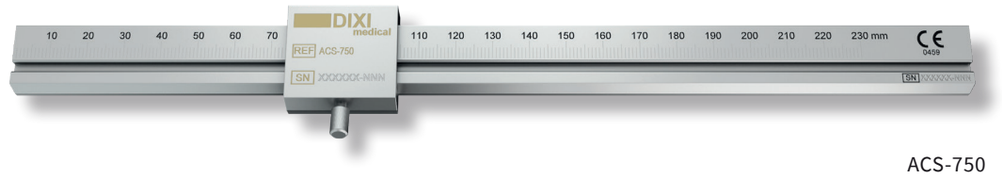

ACS-750

COAGULATION ELECTRODE & STOP
KIP-ACS-605

Class III, CE mark issued by GMED 0459
Single-use sterile material

- To coagulate the skin
- Single stop to control the depth



KIP-ACS-605

[1] *Go to page 15 to learn more.*

CH15465_MODIFICATION ROW BROCHURE PCP.indd 9 28/09/2023 11:02

IMPLANTATION TOOLS

DRILL BIT & STOP
KIP-ACS-515

Class III, CE mark issued by GMED 0459
Single-use sterile material

- Drill bit to perforate the skull with suitable diameter for the use of guiding screw
- Cutting diameter 2.1 mm
- Drill bit total length: 200 mm
- Cutting bit length: 20 mm
- Single stop to control the depth of the drill bit
- A dedicated screwdriver for securing the stop exists – ACS-714




KIP-ACS-515

COAGULATION ELECTRODE & STOP
KIP-ACS-600

Class III, CE mark issued by GMED 0459
Single-use sterile material

- To pierce and coagulate the dura mater
- Single stop to control the depth

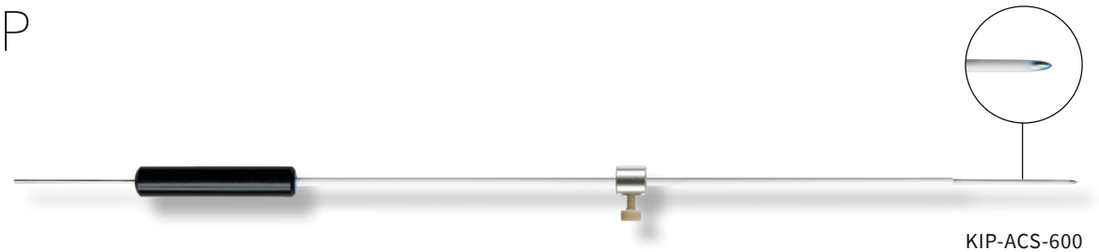

KIP-ACS-600

CH15465_MODIFICATION ROW BROCHURE PCP.indd 10 28/09/2023 11:02


IMPLANTATION TOOLS

GUIDING SCREWS
ACS-0XXSMS-10


Class III, CE mark issued by GMED 0459
Single-use sterile material

- Intended to be fixed into the bone through the skin.
- Fits through the guide tube secured to the screwdriver to optimize the placement's accuracy
- Self-tapping tip allowing a direct fixing into a hole ø 2.1 mm
- Specific threading to secure the electrode's cap to the guiding screw
- Flat area for removal using the wrench
- Individually packed, delivered per box of 10
- The guiding screws are available in 5 different lengths:
    - 15 mm - ACS-015SMS-10
    - 20 mm - ACS-020SMS-10
    - 25 mm - ACS-025SMS-10
    - 30 mm - ACS-030SMS-10
    - 35 mm - ACS-035SMS-10






ACS-015SMS-10



ACS-020SMS-10



ACS-025SMS-10



ACS-030SMS-10



ACS-035SMS-10

CH15465_MODIFICATION ROW BROCHURE PCP.indd 11 28/09/2023 11:02

IMPLANTATION TOOLS

SCREWDRIVER
ACS-710

Class I, CE mark
Delivered Non-sterile

- Long screwdriver used for the placement of guiding screw ø 2.5 mm



ACS-710

DEPTH REPORT DEVICE
ACS-751

Class Im, CE mark issued by GMED 0459
Delivered Non-sterile

- Used to measure the lenght of the DIXI medical stylet and MICRODEEP® electrode
- Unique design suitable for DIXI medical products



ACS-751

STYLET
ACS-770S-10

Class III, CE mark issued by GMED 0459
Single-use sterile material

- Used to preform the path of the electrode
- Adjustable stop integrated
- Individually packed, delivered per box of 10



ACS-770S-10

CH15465_MODIFICATION ROW BROCHURE PCP.indd 12 28/09/2023 11:02

CONNECTION CABLES CBL

CBL-XX/180

Class I, CE mark
Delivered Non-sterile

- Suitable for connecting MICRODEEP® electrodes 5 to 18 contacts
- Suitable for sterilization
- DIN connectors compatible with most EEG acquisition systems
- Overall length of 180 cm[1] for greater flexibility at the EMU and creation of damper:
  - CBL-05/180
  - CBL-08/180
  - CBL-10/180
  - CBL-12/180
  - CBL-15/180
  - CBL-18/180



[1] *Other lengths are available upon special request.*

CH15465_MODIFICATION ROW BROCHURE PCP.indd 13 28/09/2023 11:02

REMOVAL TOOLS

WRENCH FOR GUIDING SCREW REMOVAL
ACS-715

Class I, CE mark
Delivered Non-sterile

- To unlock and loosen the guiding screws
- Insert the wrench on the two flat areas of the guiding screws



ACS-715

SCREWDRIVER FOR GUIDING SCREW REMOVAL
ACS-711

Classe I, CE mark
Delivered Non-sterile

- Short screwdriver to remove the guiding screws




ACS-711

CH15465_MODIFICATION ROW BROCHURE PCP.indd 14 28/09/2023 11:02

GUIDE TUBE

The guide tube is used during SEEG procedures to accurately guide DIXI medical's SEEG instrumentation and accessories.
It provides help for the accurate placement of SEEG electrodes.
All implantation tools have an outer diameter of 2.45 mm and fit through a guide tube of min 2.5 mm.
DIXI medical manufactures three guide tubes. Most stereotactic guiding systems manufacturers provide their own guide tubes, which allow DIXI Medical's instrument to perform well, please contact your local DIXI medical representative to learn more.
The compatibility of these devices with DIXI medical's products must be checked by the physician prior to use.

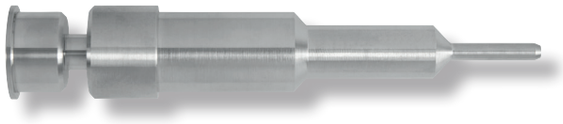

ACS-1300

Internal diameter: 2.55 mm
Variable length: 120 to 170 mm
Made of stainless steel
Sold individually with a double sterile packaging
Reusable, non-sterile



ACS-789-120

Internal diameter: 2.55 mm
Length: 120 mm
Made of stainless steel
Sold individually
Reusable, non-sterile




ACS-789-120R / ACS-789-82R*

Internal diameter: 2.55 mm
Length: 120 mm / 82.5 mm*
Made of stainless steel
Sold individually
Reusable, non-sterile

*Available end of 2023

CH15465_MODIFICATION ROW BROCHURE PCP.indd 15 28/09/2023 11:02

THERMOCOAGULATION

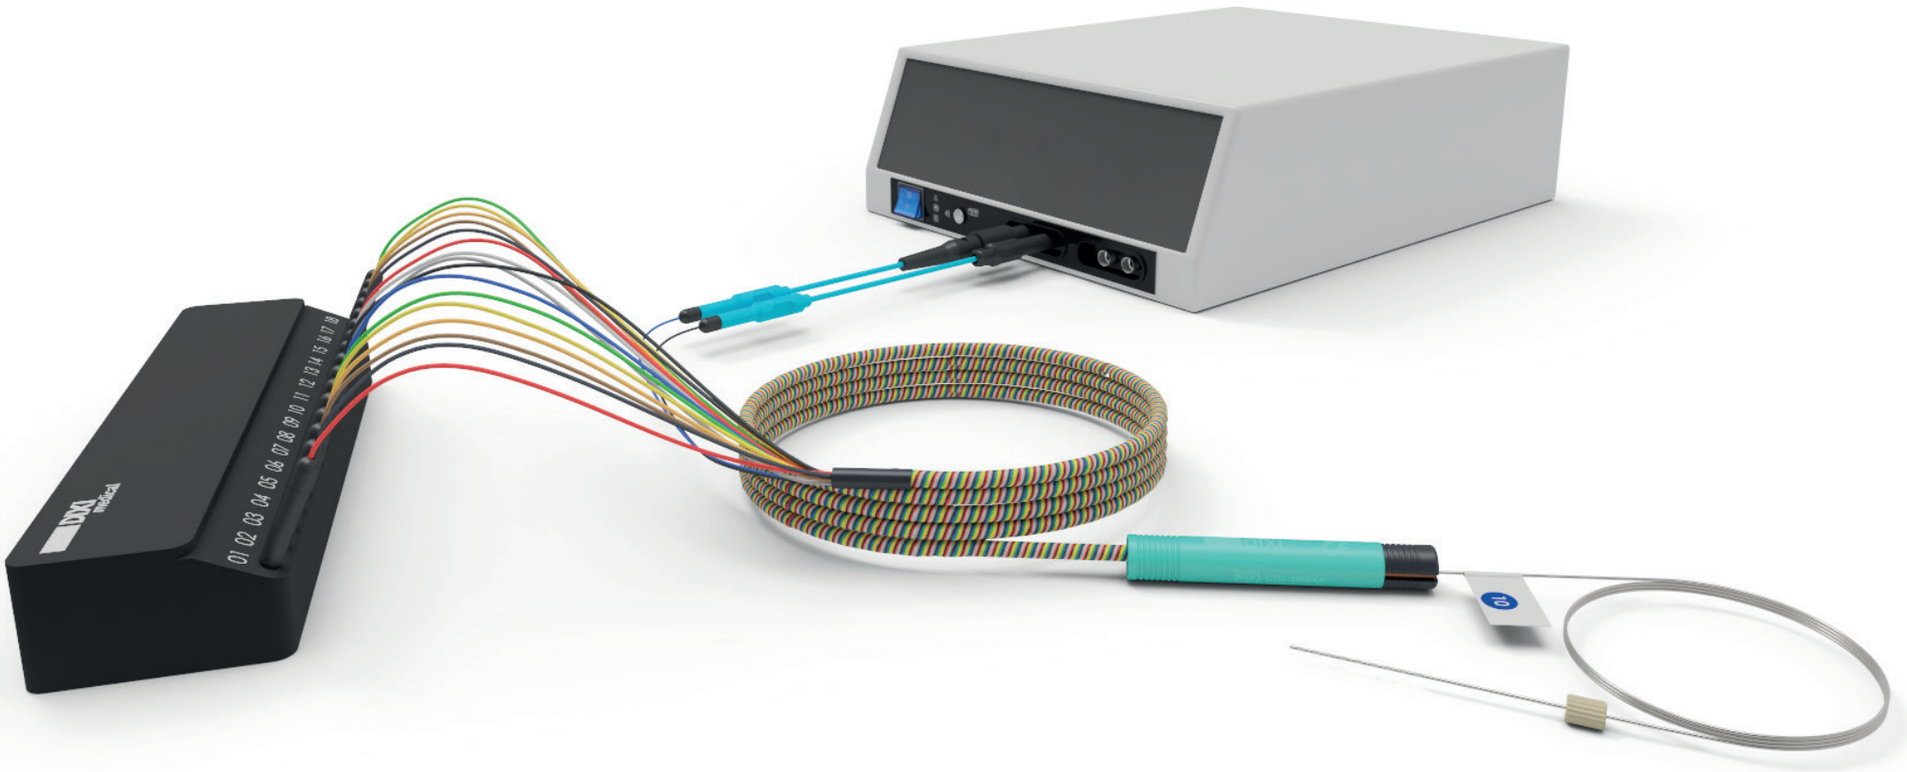

CH15465_MODIFICATION ROW BROCHURE PCP.indd 16 28/09/2023 11:02

The MICRODEEP® electrode can be used for thermocoagulation.

DIXI medical's interface cables support two radio frequency generators: Cosman G4, and INOMED N50*

INTERFACE CABLES PCP-4*0

The interface cables for use in thermocoagulation with the Microdeep® SEEG electrode are intended to connect the electrode to a compatible RF generator in order to perform a thermal lesion between two consecutive contacts.


The PCP-4*0 interface cables come with a preparation box and must be used with a CBL cable. For more information on the connection, scan the QR code below.

INTERFACES

The PCP-4*0 can be connected to two generators:

- Cosman G4 (PCP-410)
- INOMED N50 (PCP-420)

SCAN
TO WATCH
THE VIDEO

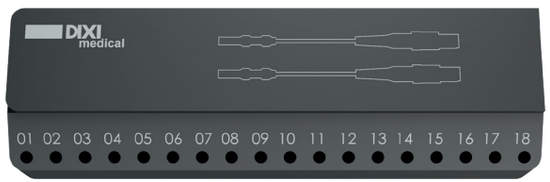



PCP-410
(Cosman G4)



PCP-420
(INOMED N50)

Check the availability of thermocoagulation with your local representative.

Thermocoagulation can also be performed with the INOMED LG2-SEEG system. Please contact your INOMED representative to learn more.


DIXI medical

CH15465_MODIFICATION ROW BROCHURE PCP.indd 17 28/09/2023 11:02

INTRAOPERATIVE CORTEX STRIP/ GRID ELECTRODES

WITH CONNECTION CABLES

The intraoperative solution
for brain mapping and stimulation

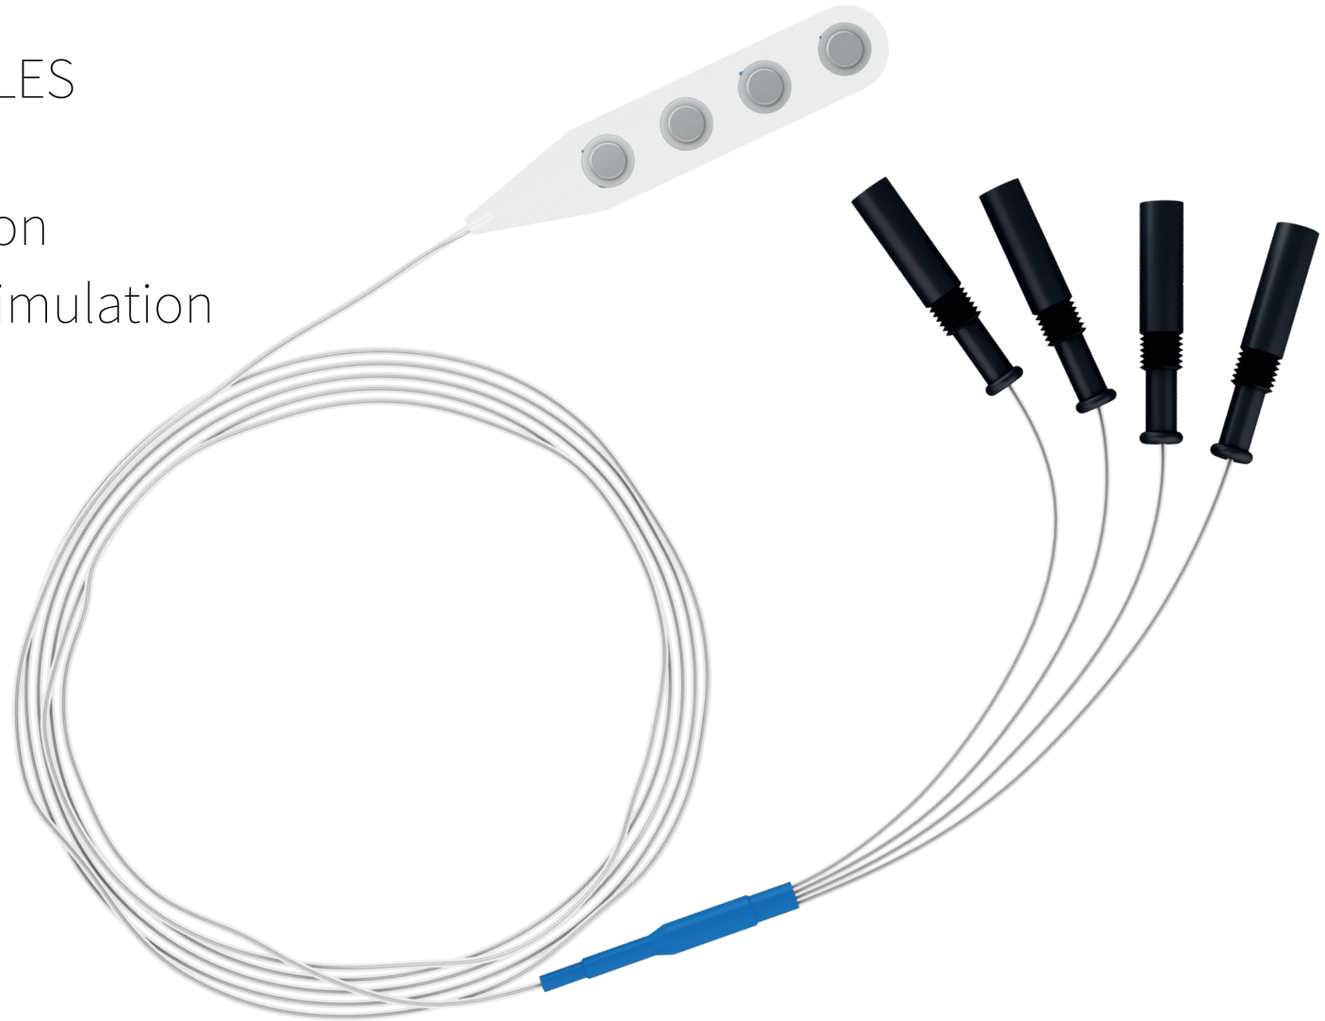


Classe III, CE mark issued by GMED 0459

Single-use sterile material

CH15465_MODIFICATION ROW BROCHURE PCP.indd 18 28/09/2023 11:02

- Thin <0.8 mm and flexible to be as close as possible to brain tissue
- Contacts made of stainless steel
- Contacts useful diameter: 4 mm
- Distance between the contacts: 10 mm
- Width of strips: 10 mm
- Numbered contacts
- Dome shaped contacts
- Micro-perforations in between strips
- Built-in Touch-Proof connectors (DIN 42802) to ensure ease of use in the OR and compatibility with most acquisition and stimulation systems
- Contacts number engraved on the DIN
- Cable length : 2 m

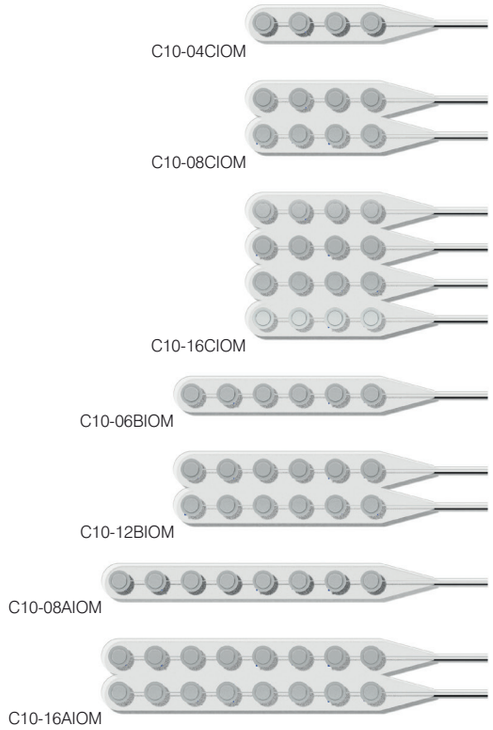


CH15465_MODIFICATION ROW BROCHURE PCP.indd 19 28/09/2023 11:02

MICRODEEP®

5 contacts	D08-05AM
8 contacts	D08-08AM
10 contacts	D08-10AM
12 contacts	D08-12AM
15 contacts	D08-15AM
15 contacts	D08-15BM
15 contacts	D08-15CM
18 contacts	D08-18AM
18 contacts	D08-18CM

CONNECTION CABLES CBL

5 contacts	CBL-05/180
8 contacts	CBL-08/180
10 contacts	CBL-10/180
12 contacts	CBL-12/180
15 contacts	CBL-15/180
18 contacts	CBL-18/180

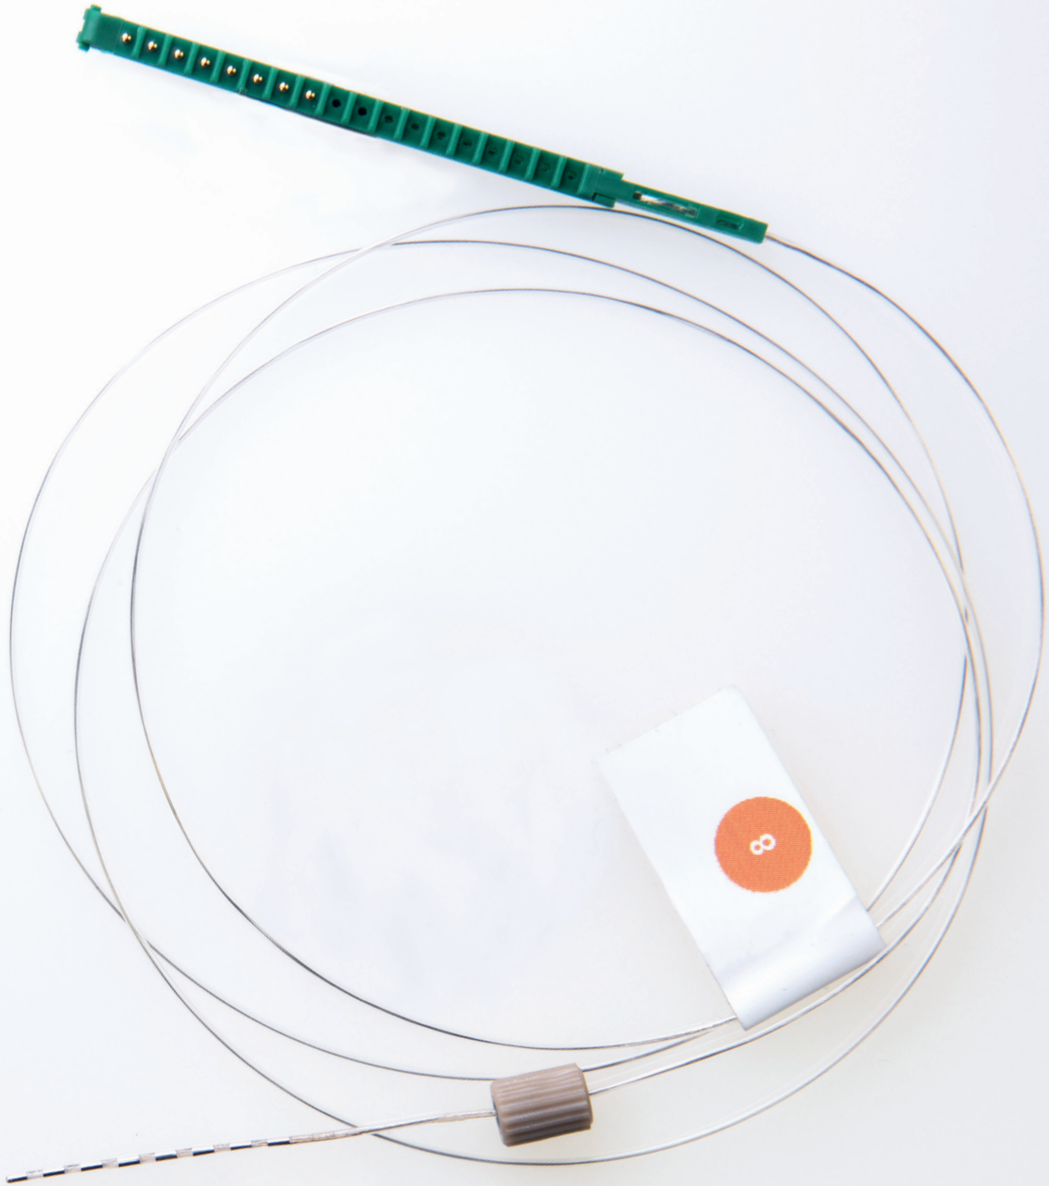

CH15465_MODIFICATION ROW BROCHURE PCP.indd 20 28/09/2023 11:02

SINGLE USE IMPLANTATION TOOLS

Coagulation electrode & Stop (dura-mater)	KIP-ACS-600
Coagulation electrode & Stop (skin)	KIP-ACS-605
Drill bit & Stop (140 mm)	KIP-ACS-510
Drill bit & Stop (200 mm)	KIP-ACS-515
Guiding screws 15 mm	ACS-015SMS-10
Guiding screws 20 mm	ACS-020SMS-10
Guiding screws 25 mm	ACS-025SMS-10
Guiding screws 30 mm	ACS-030SMS-10
Guiding screws 35 mm	ACS-035SMS-10
Stylet	ACS-770S-10
Caps	ACS-050S-5

REUSABLE REMOVAL TOOLS

Short screwdriver	ACS-711
Wrench	ACS-715

REUSABLE IMPLANTATION TOOLS

Bone starter	ACS-745
Long screwdriver	ACS-710
Screwdriver for stop	ACS-714
Sliding ruler	ACS-750
Depth report device	ACS-751
Single stop	ACS-760
Marking rod & Stop	ACS-740

CH15465_MODIFICATION ROW BROCHURE PCP.indd 21 28/09/2023 11:02

DIXI medical support

DIXI medical supports hospitals worldwide to provide the best experience using our devices. We guide you from the first order through a dry-run to your first surgeries. The clinical support team is at your disposal to answer all your questions and concerns.

We take a lot of pride in manufacturing high-quality devices, and we want to provide you with the best service. Our Quality Affairs department handles your complaints and conducts thorough investigations to ensure it never happens again.

The Regulatory Affairs landscape is rapidly evolving, and this is why our capacities increased to properly answer in the best way possible the new demands from authorities.

Innovation also lies in DIXI medical's DNA. Our R&D team and the DIXI neurolab are constantly looking to improve and develop new technologies. Stay tuned!

We thank you for your confidence over the past 40 years and are pleased to count you as one of our contributors.

CH15465_MODIFICATION ROW BROCHURE PCP.indd 22 28/09/2023 11:02






DIXI medical
CH15465_MODIFICATION ROW BROCHURE PCP.indd 23 28/09/2023 11:02




+33.381.889.890

info@diximedical.com

www.diximedical.com

PC_007_R01

CH15465_MODIFICATION ROW BROCHURE PCP.indd 24 28/09/2023 11:02